PATENT ABSTRACTS OF JAPAN

(11)Publication number:

07-260719

(43) Date of publication of application: 13.10.1995

(51)Int.CI. G01N 24/00
G01R 33/20
G01V 3/14

(21)Application number: 06-071302 (71)Applicant: HITACHI MEDICAL CORP


(22)Date of filing: 17.03.1994 (72)Inventor: NAGASAWA YASUO

(54) NUCLEAR QUADRUPOLE RESONANCE APPARATUS

(57) Abstract:

PURPOSE: To enable execution of a switching operation at a time point when a residual voltage due to an NQR excitation pulse is attenuated to 1/n of the one according to a usual method, in a switching circuit for cutting off a high-frequency pulse amplifier from a high-frequency coil and a measuring circuit after completion of the excitation pulse and connecting a lo noise amplifier to the high-frequency coil.

CONSTITUTION: In regard to an impedance matching circuit of a high-frequency coil, the circuit is so constructed that a high-frequency pulse input circuit has a value larger (in (n) times) than an output impedance of an NQR signal measuring circuit, and a high-frequency amplifier and a diode for switching it are connected to the aforesaid circuit. Since the high-frequency amplifier is cut off at a time point when a residual voltage due to a pulse for NQR excitation becomes 1/n of the one according to a prior art, a time for attenuation of the residual voltage is shortened, while the residual voltage contained in an input signal to a low-noise amplifier can be reduced to 1/n.



LEGAL STATUS

[Date of request for examination]

[Date of sending the examiner's decision of rejection]

[K': d of final disposal of application other than the ex ...iner's decision of rejection or application converted registration]

[Date of final disposal for application]

[Patent number]


[Date of registration]

[Number of appeal against examiner's decision of rejection]

[Date of requesting appeal against examiner's decision of rejection]

[Date of extinction of right]

Copyright (C); 1998,2003 Japan Patent Office

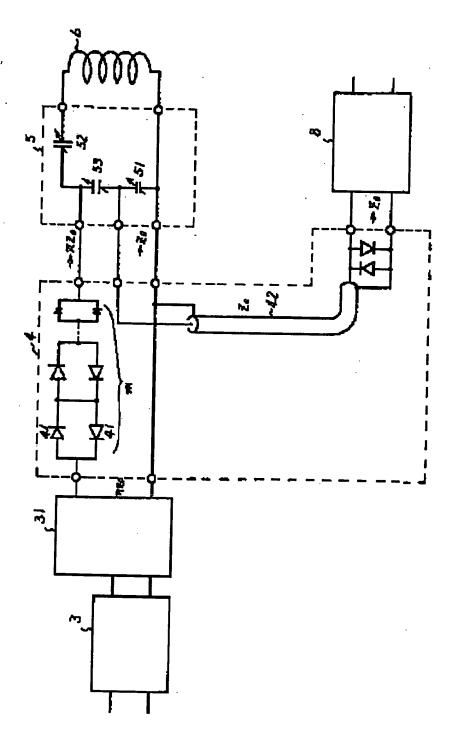

★HITR S01 S03 96-001798/01 ★JP 07260719-A

Nuclear quadrupole resonance device for narcotics detection - has switching circuit which switches off input/output of high frequency coil, when residual voltage is attenuated to 1/n value by excitation pulse

I IΓΓΑCI II MEDICAL CORP 94.03.17 94JP-071302 W06 (95.10.13) G01N 24/00, G01R 33/20, G01V 3/14

The NQR device has a switching circuit (4) which connects a high frequency coil (6) with a pulse amplifier (3) and a low noise amplifier (8). The output impedance of the pulse input circuit is higher than the output impedance of the NQR signal measurement circuit.

The switching circuit has a number of diodes arranged between the tuning circuit (5) and the pulse amplifier. When the residual voltage of excitation pulse attenuates to 1/nth of it, the switching circuit switches off the input/output high frequency coil.

ADVAN TAGE - Shortens decay time of residual voltage. Improves mixing of residual signal with low noise amplifier. (6pp Dwg.No.3/4)
No. 001546